

PAPP-A [¹²⁵I] IRMA kit (REF: RK-4CT)

The ¹²⁵I-PAPP-A IRMA system provides direct quantitative *in vitro* determination of pregnancy-associated plasma protein A in human serum, in the range of 0-45 µg/ml. Each kit contains material sufficient for 100 determinations, permitting the construction of one standard curve and the assay of 42 unknowns in duplicate.

Introduction

Pregnancy-associated plasma protein A is a large placenta-derived glycoprotein. The biological function of PAPP-A is not completely known, it has been shown its proteolytic and immuno-regulating action through cleavage of insulin-like growth factor binding protein 4.

PAPP-A maternal serum concentration rises during pregnancy. Mostly, values under 0.5 MOM (multiple of median) are considered pathological, however, isolated PAPP-A data have no diagnostic value by itself.

This kit can be used in the risk assessment of Down's Syndrome (Trisomy 21) in combination with other biochemical and ultrasound parameters as specified above, taking also into account other data like maternal age and weight and using a validated software for Down's Syndrome risk assessment (*see Annex*):

- Combined test:** maternal serum PAPP-A and free-βhCG determination and nuchal translucency (NT) thickness measurement by an ultrasound scan in the first trimester of pregnancy.
- Integrated test:** maternal serum PAPP-A determination and nuchal translucency (NT) thickness measurement by an ultrasound scan in the first trimester of pregnancy and maternal serum AFP, hCG, unconjugated Estriol and Inhibin-A determination in the second trimester.

Principle of method

This technology uses two high affinity monoclonal antibodies in an immunoradiometric assay (IRMA) system. The ¹²⁵I labelled signal-antibody binds to an epitope of the PAPP-A molecule spatially different from that recognized by the biotin-capture-antibody. The two antibodies react simultaneously with the antigen present in standards or samples, which leads to the formation of a capture antibody - antigen - signal antibody complex, also referred to as a "sandwich". During 2-hours incubation period with shaking, immuno-complex is immobilized to the reactive surface of streptavidin coated test tubes. Reaction mixture is then discarded, test tubes washed exhaustively, and the radioactivity is measured in a gamma counter.

The concentration of antigen is directly proportional to the radioactivity measured in test tubes. By constructing a calibration curve plotting binding values against a series of

calibrators containing known amounts of PAPP-A, the unknown concentration of PAPP-A in patient samples can be determined.

Contents of the kit

- 1 bottle TRACER (21 ml), ready to use, containing about 740 kBq ¹²⁵I-anti-PAPP-A and capture anti-PAPP-A antibody in buffer with red dye and 0.1 % NaN₃.
- 6 vials STANDARD (6 x 0.4 ml), ready to use, containing (S1-S6): 0, 0.45, 1.35, 4.5, 13.5, 45 µg/ml (1 IU/l = 4.5 µg/ml) in serum with 0.1% Kathon CG. *In the absence of an international reference preparation, standards have been prepared gravimetrically using highly pure (>99%) PAPP-A (FITZGERALD 30AP66)*
- 2 vials of CONTROL SERUM (2 x 0.4 ml), ready to use, containing 0.1% Kathon CG. The concentration of the control serum is specified in the quality certificate enclosed.
- 2 boxes COATED TUBE, ready to use. 2x50 reactive test tubes, 12x75 mm, packed in plastic boxes.
- 1 bottle WASH BUFFER CONCENTRATE (20 ml), containing 0.1% NaN₃. See *Preparation of reagents*.

Quality certificate

Pack leaflet

Materials, tools and equipment required

Test tube rack, precision pipettes with disposable tips (10, 200 and 2000 µl), distilled water, vortex mixer, shaker, plastic foil, absorbent tissue, gamma counter.

Recommended tools and equipment

Repeating pipettes (e.g. Eppendorf or else), dispenser with 1-L reservoir (instead of the 2-ml pipette).

Specimen collection and storage

Serum samples can be prepared according to common procedures used routinely in clinical laboratory practice. Samples can be stored at 2-8 °C if the assay is carried out within 24 hours, otherwise aliquots should be prepared and stored deep frozen (-20°C). Frozen samples should be thawed and thoroughly mixed before assaying. Avoid repeated freezing-thawing cycles of samples. Hemolyzed and lipemic specimens may give false values and should not be used.

Preparation of reagents, storage

Add the wash buffer concentrate (20 ml) to 700 ml distilled water to obtain 720 ml wash solution. After dilution, store at 2-8°C until expiry date of the kit.

Store the rest of reagents between 2-8°C after opening. At this temperature each reagent is stable until expiry date of the kit. The actual expiry date is given on the package label and in the quality certificate.

CAUTION!

Equilibrate all reagents and serum samples to room temperature. Mix all reagents and samples thoroughly before use. Avoid excessive foaming.

Assay procedure

(For a quick guide, refer to Table 1.)

- Label coated tubes in duplicate for each standard (S1-S6), control serum and sample.
- Homogenize all reagents and samples by gentle mixing to avoid foaming.
- Pipette 10 µl of standards, control and samples into the properly labeled tubes. Use rack to hold the tubes. Do not touch or scratch the inner bottom of the tubes with pipette tip.
- Pipette 200 µl of tracer into each tube.
- Seal all tubes with a plastic foil. Fix the test tube rack firmly onto the shaker plate. Turn on the shaker and adjust an adequate speed such that liquid is constantly rotating or shaking in each tube.
- Incubate tubes for 2 hours, shaking at room temperature.
- Add 2.0 ml of diluted wash buffer to each tube. Decant the supernatant from all tubes by the inversion of the rack. In the upside down position place the rack on an absorbent paper for 2 minutes.
- Return the tube-rack to an upright position, and repeat step-7 two more times.
- Count each tube for at least 60 seconds in a gamma counter.
- Calculate the PAPP-A concentrations of the samples as described in calculation of results or use special software.

Table 1. Assay Protocol, Pipetting Guide (all volumes in microlitres)

Tubes	Total	Standard	Control	Sample
Standard		10		
Control			10	
Sample				10
Tracer	200	200	200	200
Shake for 2 hours at room temperature				
Wash buffer		2000	2000	2000
Decant the fluid and blot on filter paper				
Wash buffer		2000	2000	2000
Decant the fluid and blot on filter paper				
Wash buffer		2000	2000	2000
Decant the fluid and blot on filter paper				
Count radioactivity (60 sec/tube)				
Calculate the results				

Calculation of results

The calculation is illustrated using representative data. The assay data collected should be similar to those shown in Table 2.

Calculate the average count per minute (CPM) for each pair of assay tubes.

Calculate the normalized percent binding for each standard, control and sample respectively by using the following equation:

$$B/T(\%) = \frac{S_{2-6} / C / M_x (\text{cpm}) - S_1 (\text{cpm})}{T(\text{cpm})} \times 100$$


Using semi-logarithmic graph paper plot B/T (%) for each standard versus the corresponding concentration of PAPP-A.

Determine the PAPP-A concentration of the unknown samples by interpolation from the standard curve. Do not extrapolate values beyond the standard curve range.

Out of fitting programs applied for computerized data processing, logit-log or spline fittings can be used. Automated data processing systems are also available.

Table 2. Typical assay data

Tubes	Count cpm	Mean cpm	B/T%
T	324642 330422	327532	-
S1	73 101	87	0.03
S2	2564 2627	2564	0.76
S3	7583 7386	7485	2.26
S4	25131 24176	24654	7.50
S5	71400 69580	70490	21.55
S6	178872 180902	179887	54.90
C1	35452 37484	36468	11.11
C2	68212 64829	66520	20.28

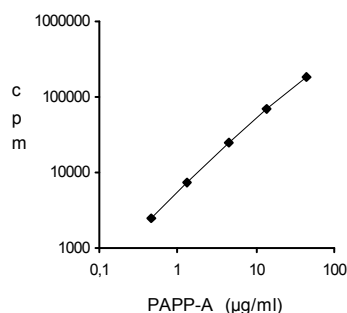

1. ábra

Figure 1: A typical standard curve
(Do not use to calculate unknown samples)

Characterization of assay

Typical assay parameters

Bmax/T > 40%
NSB/T < 0.1%

Sensitivity

The analytical sensitivity is 0.0143 µg/ml, obtained by assaying 15 replicates of the zero standard. The sensitivity has been determined as the concentration corresponding to the sum of the mean cpm and its double standard deviation.

Dilution test (linearity)

Five samples were measured in a series of dilution with zero-standard. The following equation obtained for measured (Y) versus expected (X) concentration demonstrates the good linearity:

$$Y = 1.047x - 0.08 \quad R = 0.9995 \quad n = 25$$

Precision and reproducibility

Seven patient samples were assayed in 15 replicates to determine intra-assay precision. To determine inter-assay precision seven patient samples were measured in duplicates in 22 independent assays using different kit batches. Values obtained are shown below.

Intra-assay		Inter-assay	
Mean (µg/ml)	CV %	Mean (µg/ml)	CV %
6.57	6.20	6.75	2.80
12.31	1.68	12.74	2.73
1.91	4.07	1.82	3.07
4.11	4.69	4.04	2.98
7.04	4.12	6.96	3.84
15.06	4.51	15.53	3.82
27.47	3.49	27.43	2.88

Recovery

Recovery was defined as the measured increase expressed as per cent of expected increase upon spiking serum samples with known amounts of PAPP-A. The average per cent recovery for five serum pools spiked with PAPP-A at four levels was: $99.4 \pm 3.3\%$ (mean \pm SD).

Hook effect

The KIT has no "high-dose hook" effect with PAPP-A levels up to 800 µg/ml. Samples expected to have concentrations greater than the highest standard should be diluted with the zero standard and reassayed.

Expected Values

Pregnancy weeks	1MOM (µg/ml)	N
10	8.92	22
11	10.51	500
12	14.75	1833
13	20.54	775

It is recommended that each laboratory determine a reference range for its own patient population. The results of this assay should be used in conjunction with other pertinent clinical information.

Every three months MoM values should be checked and, if necessary, recalculated.

Procedural notes

1) **Source of error!** Reactive test tubes packed in plastic boxes are not marked individually. Care should be taken of not mixing them with common test tubes. To minimize this risk, never take more tubes than needed out of plastic box, and put those left after work back to the box. It is recommended to label assay tubes by a marker pen.

2) **Source of error!** To ensure the efficient rotation, tubes should be firmed tightly inside the test tube rack. Never use a rack type with open hole. An uneven or incomplete shaking may result in a poor assay performance.

3) **Addition of wash buffer.** For the addition of wash buffer the use of a common laboratory dispenser equipped with a 1-L glass bottle, and a flexible outlet tubing end is recommended. In lack of this tool a large-volume syringe attached to a repeating pipette can be used.

Additional information

Components from various lots or from kits of different manufacturers should not be mixed or interchanged.

Precaution

Radioactivity

This product contains radioactive material. It is the responsibility of the user to ensure that local regulations or code of practice related to the handling of radioactive materials are satisfied.

Biohazard

Human blood products used in the kit have been obtained from healthy human donors. They were tested individually by using approved methods (EIA, enzyme immunoassay), and were found to be negative, for the presence of both Human Immunodeficiency Virus antibody (Anti-HIV-1) and Hepatitis B surface Antigen (HBsAg). Care should always be taken when handling human specimens to be tested with diagnostic kits. Even if the subject has been tested, no method can offer complete assurance that Hepatitis B Virus, Human Immunodeficiency Virus (HIV-1), or other infectious agents are absent. Human blood samples should therefore be handled as *potentially infectious materials*.

Chemical hazard

Some components contain sodium azide as an antimicrobial agent. Dispose of waste by flushing with copious amount of water to avoid build-up of explosive metallic azides in copper and lead plumbing. The total azide present in each pack is 41 mg. Some components contain Kathon CG as an antimicrobial agent. The total Kathon CG present in each pack is 3.2 mg.

	Use by	CONTROL	Control
LOT	Batch code	CAL	Standard
	Caution, consult accompanying documents	CT	Coated tube
	Biological risk	TRAC	Tracer
	Consult operating instructions	WASHB	Wash buffer
IVD	In vitro diagnostic medical device		Temperature limitation Store between 2-8°C
	Manufacturer		Radioactive Material
REF	Catalogue number		

CE1011

Website: <http://www.izotop.hu>

Technical e-mail: immuno@izotop.hu

Commercial e-mail: commerce@izotop.hu

IZOTOP

INSTITUTE OF ISOTOPES Ltd.

1535 Budapest. Pf.: 851.

Tel.: (36-1)392-2577, Fax: (36-1)395-9247

Edition: June 2011

Annex to the Instructions for Use

In vitro kits for Down's Syndrome risk assessment

This kit has been validated for the risk assessment of 21 Trisomy, using the following kits and software:

Kit / software name	Code	Manufacturer
PAPP-A IRMA	RK-4 CT	Institute of Isotopes Ltd.
Free β hCG IRMA	RK-820CT	Institute of Isotopes Ltd.
AFP IRMA	RK-800 CT	Institute of Isotopes Ltd.
hCG RIA	RK-770 CT	Institute of Isotopes Ltd.
Unconjugated Estriol RIA	RK-3 CT	Institute of Isotopes Ltd.
Active Inhibin-A ELISA	DSL-10-28100	DSL - Beckman Coulter
alpha - Antenatal Screening Software for Down's Syndrome and Neural Tube Defects.		Logical Medical Systems Ltd.

The kits and software listed before are CE marked. They can be used together for the risk assessment of Trisomy 21, according to the 98/79 EC IVD directive and based on the conformity assessment performed by an authorized notified body (CE1011).

Resumed results of validation, regarding efficiency of risk assessment:

Sensitivity

Screening method	Number of tests performed	Positive cases with the test		Cases confirmed by cytogenetic test		Fals positive cases	
		No.	%	No.	% of positive tests	No.	%
Combined Test	1389	42	3,02	2	4,76	40	2,88
Quadruple Test	539	30	5,57	1	3,33	29	5,38
Integrated Test	1741	47	2,70	3	6,38	44	2,53

Specificity

Screening method	Number of tests performed	Negative cases	Negative cases with the test		Fals negative cases
			No.	%	No. (%)
Combined Test	1389	1387	1345	96,97	1 (0,07)
Quadruple Test	539	538	508	94,42	0
Integrated Test	1741	1738	1691	97,30	0

Literature: see www.izotop.hu

CE₁₀₁₁

WEB site: <http://www.izotop.hu>

Technical e-mail: immuno@izotop.hu

Commercial e-mail: commerce@izotop.hu



INSTITUTE OF ISOTOPES Ltd.

1535 Budapest. Pf.: 851.

Tel.: +36 1 392-2577, Fax: +36 1 395-9247